



PHARMA DEVILS


QUALITY ASSURANCE DEPARTMENT


LOADED CHAMBER HEAT PENETRATION STUDIES


LOAD PATTERN : MAXIMUM LOAD

CYCLE NO. : 1

LOAD : STERILITY TEST MEDIA TUBES

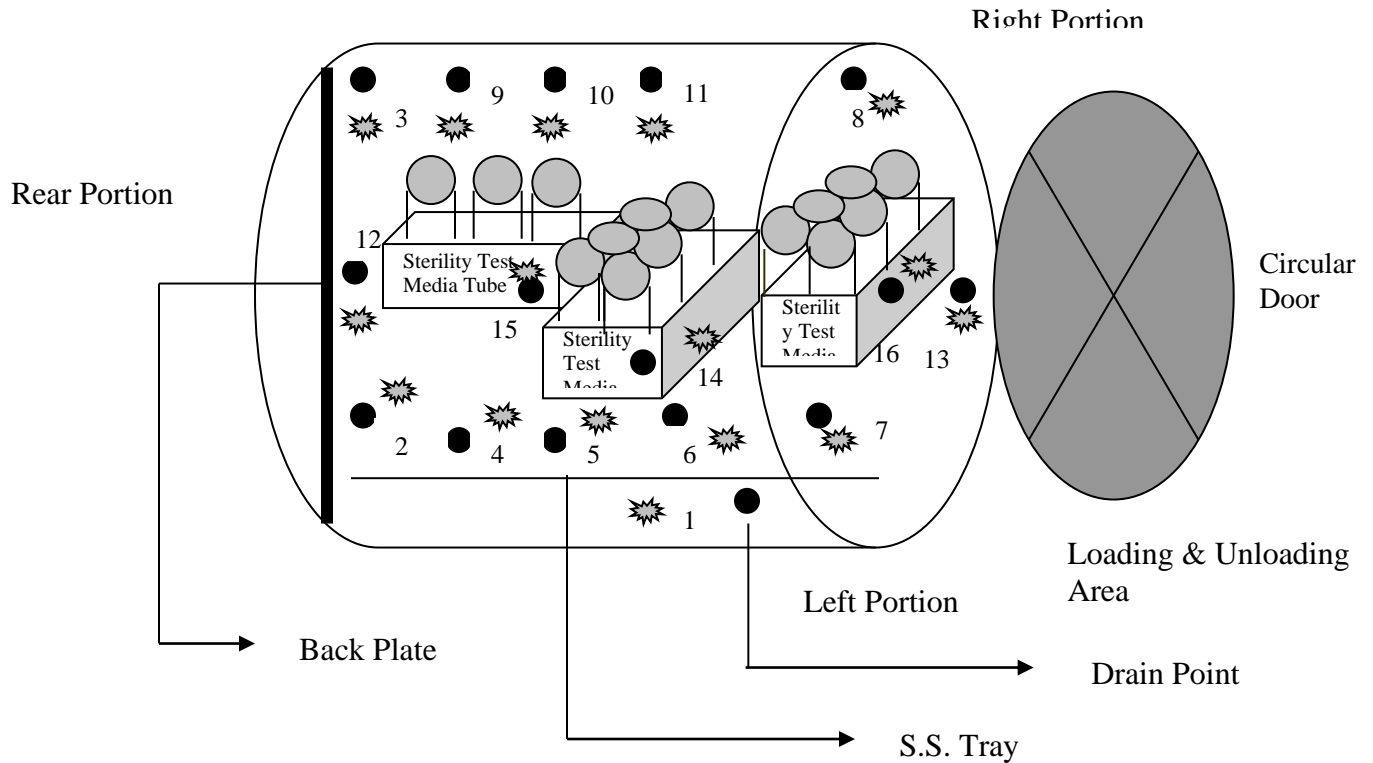

Biological Indicator: 

RTD Probes: 

**LOCATIONS OF BIOLOGICAL INDICATORS AND PROBES
DURING LOADED CHAMBER HEAT PENETRATION**